



2015 NCIMS Proposal 211

DRAFT Pilot Program Accepted Tetracycline Test Kit Using Both Undiluted and Diluted Steps


PRESUMPTIVE POSITIVE DETERMINATION

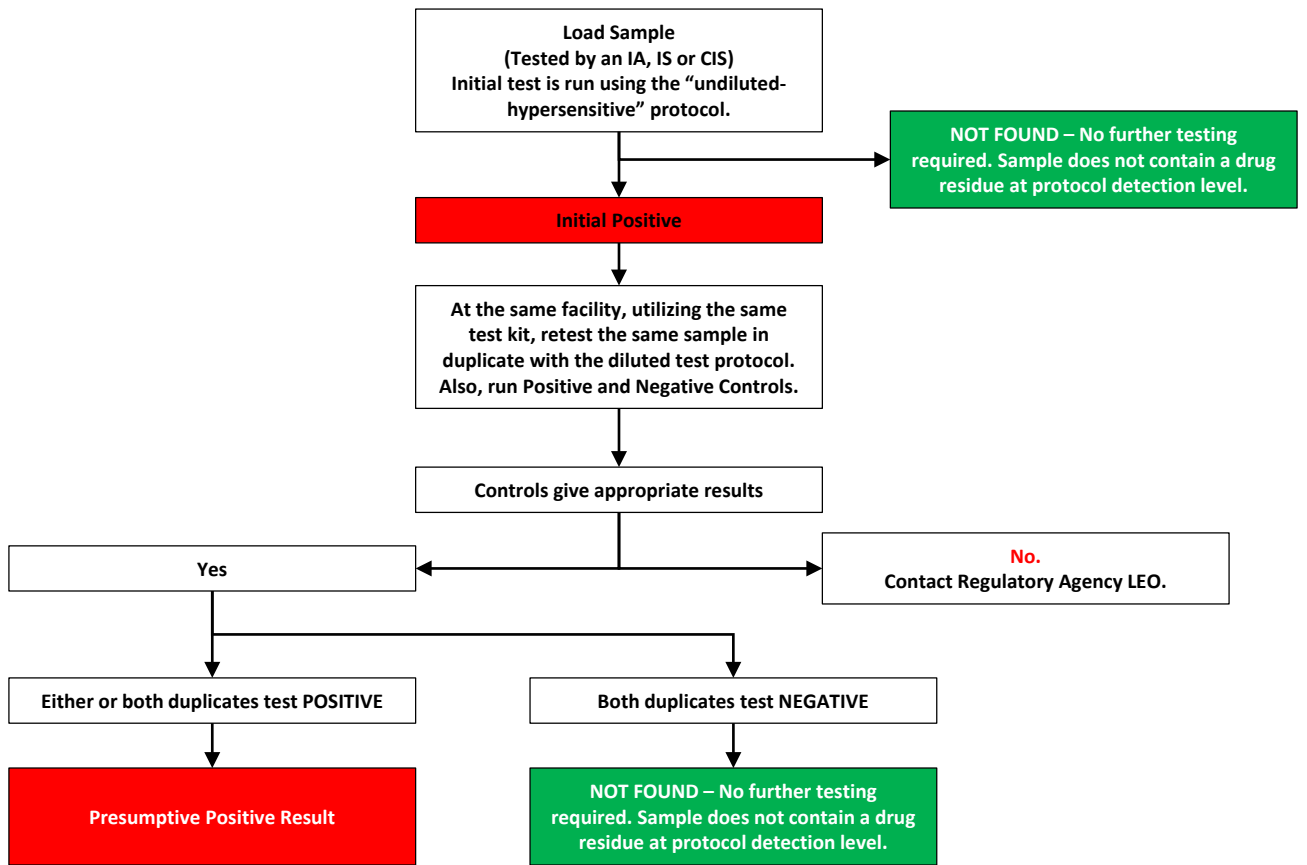

CONFIRMATION OF POSITIVE

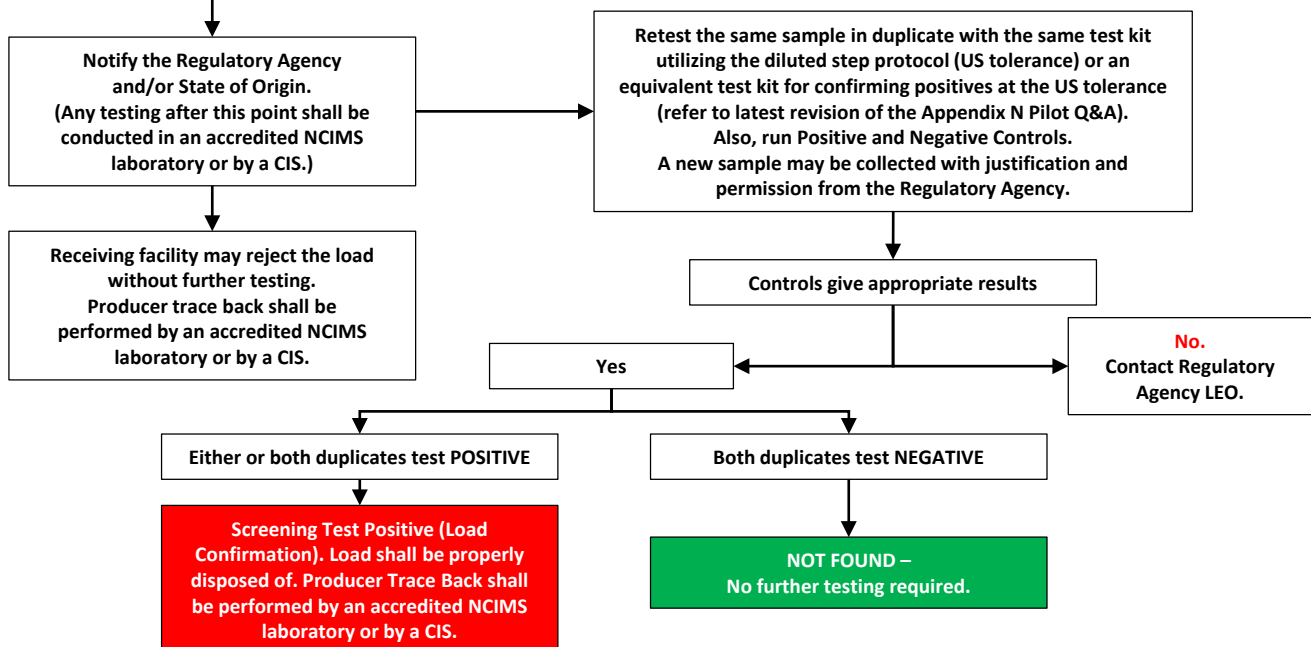

TETRACYCLINE PRODUCER TRACE BACK

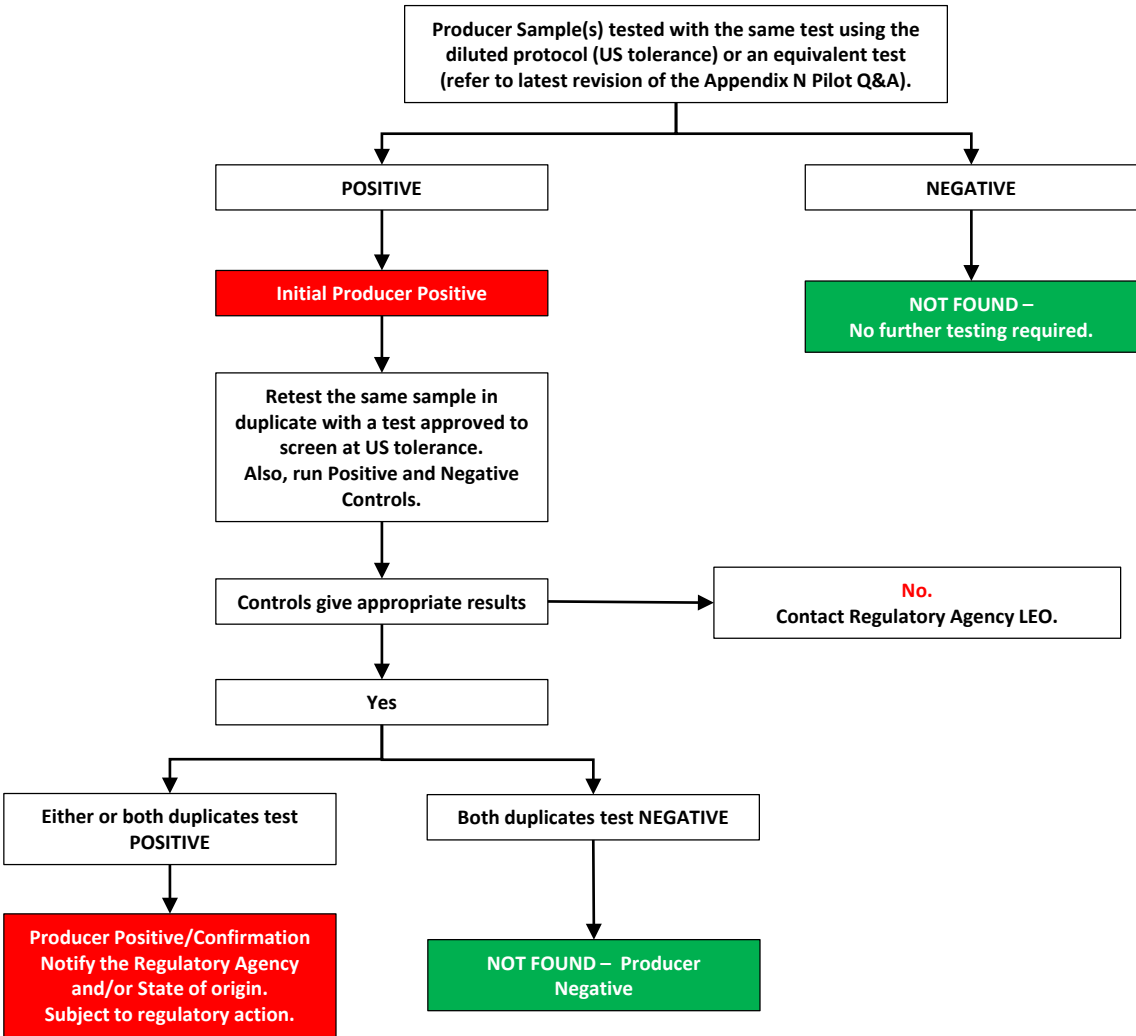

Note: Suspension of permit or equally effective measures shall immediately be taken to prevent the sale of milk containing drug residues and further pickup or use of milk shall be immediately discontinued.

PRODUCER REINSTATEMENT

Producers that test Positive shall have a Negative sample using the diluted protocol (US tolerance) or an equivalent test (refer to latest revision of the Appendix N Pilot Q&A).

Note: CVM will allow a kit for use in the NCIMS Proposal 211 Pilot testing for tetracyclines to test for oxytetracycline and either chlortetracycline or tetracycline at the published tolerance (300 ppb). However, for the drug (tetracycline or chlortetracycline) that is not detected at the tolerance, the 90/95 must be within twice the tolerance (600 ppb).